

METHOD AND APPARATUS FOR
CONTROLLING POSITION OF A LASER
OF A MALDI MASS SPECTROMETER

James P. Reilly et al.
32993-72728/ARTI-0335-A

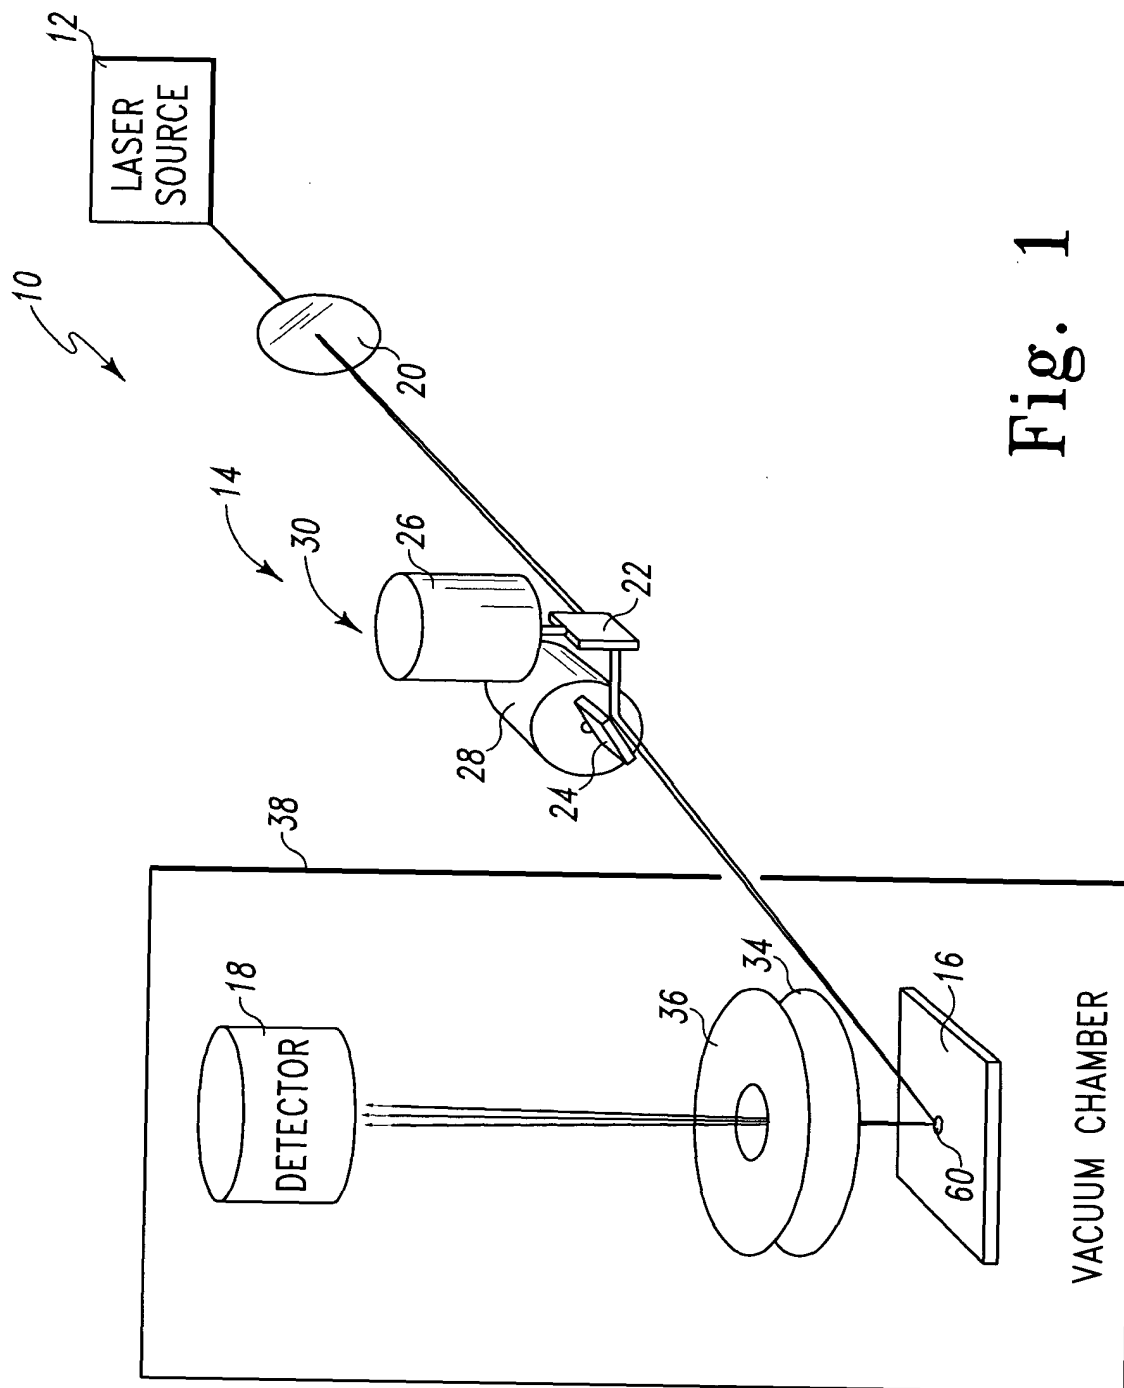


Fig. 1

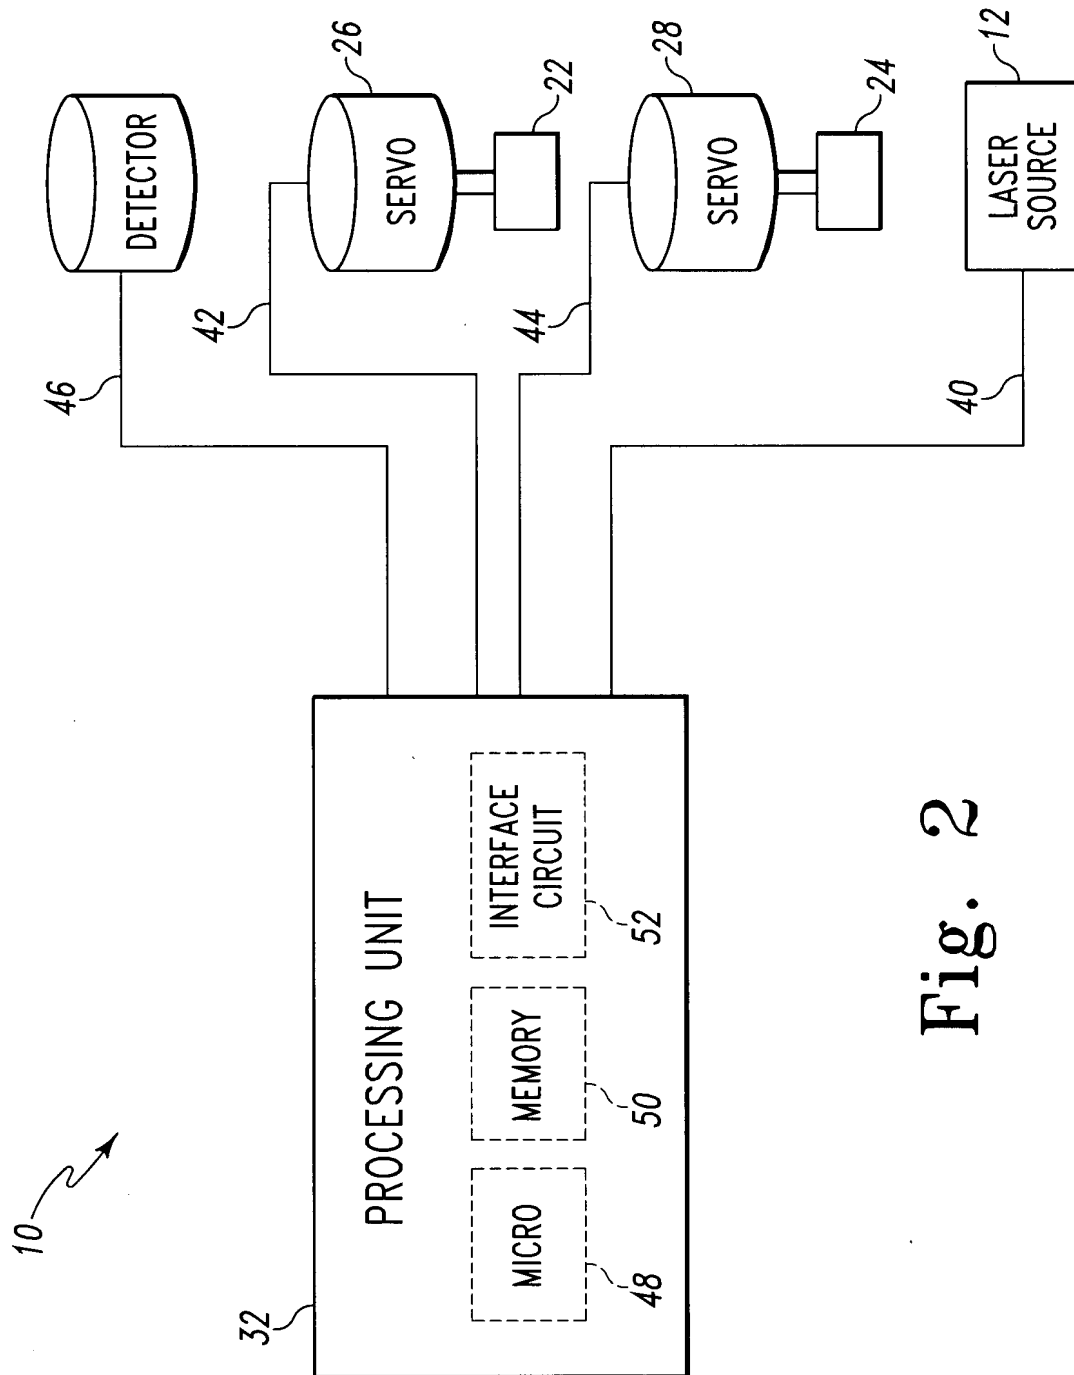


Fig. 2

METHOD AND APPARATUS FOR
CONTROLLING POSITION OF A LASER
OF A MALDI MASS SPECTROMETER

James P. Reilly et al.
32993-72728/ART1-0335-A

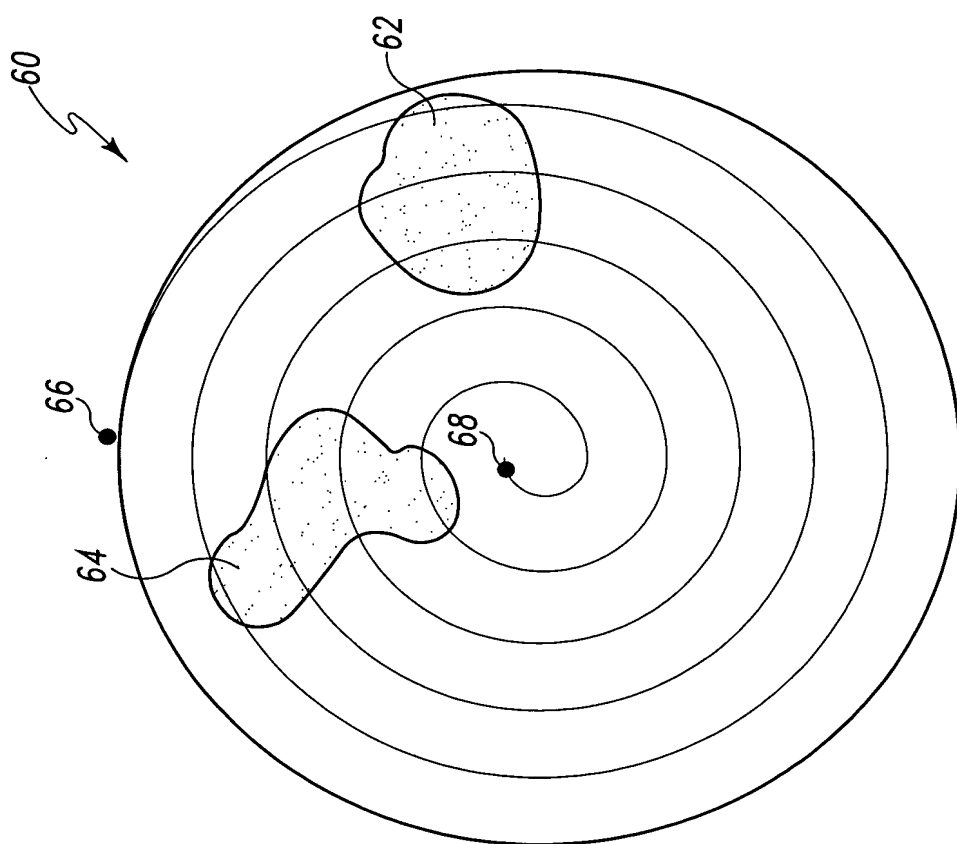


Fig. 3

Fig. 4

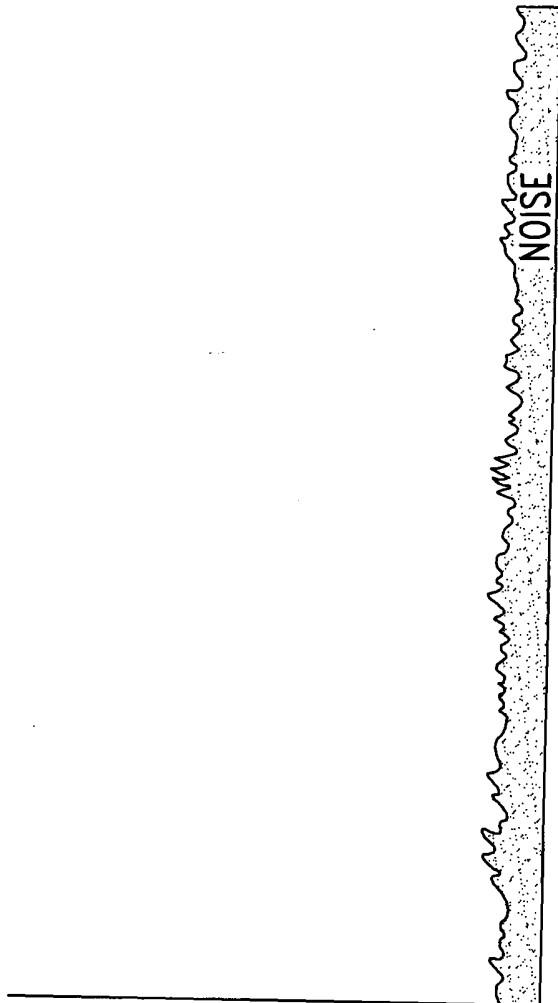


Fig. 5

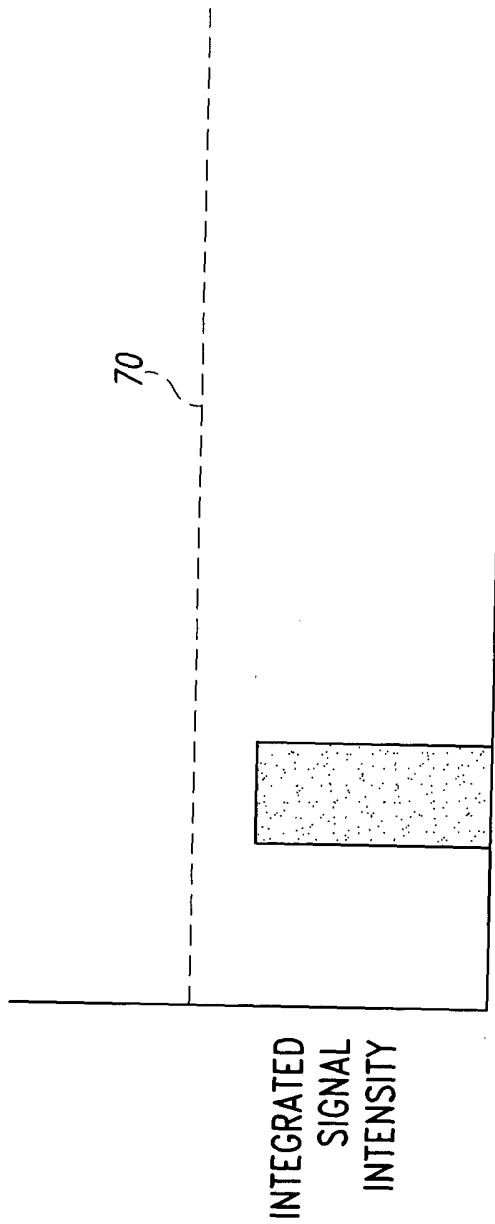


Fig. 6

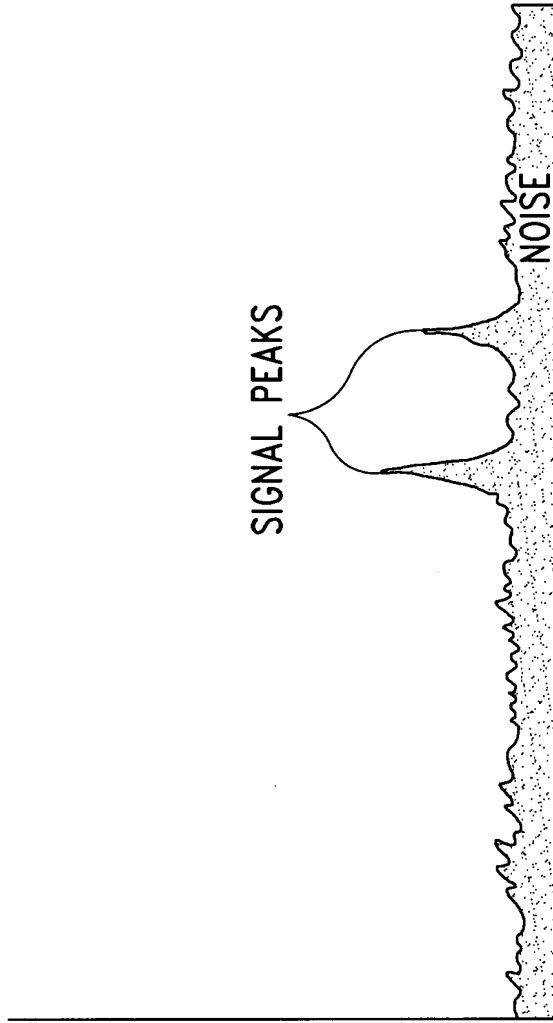


Fig. 7

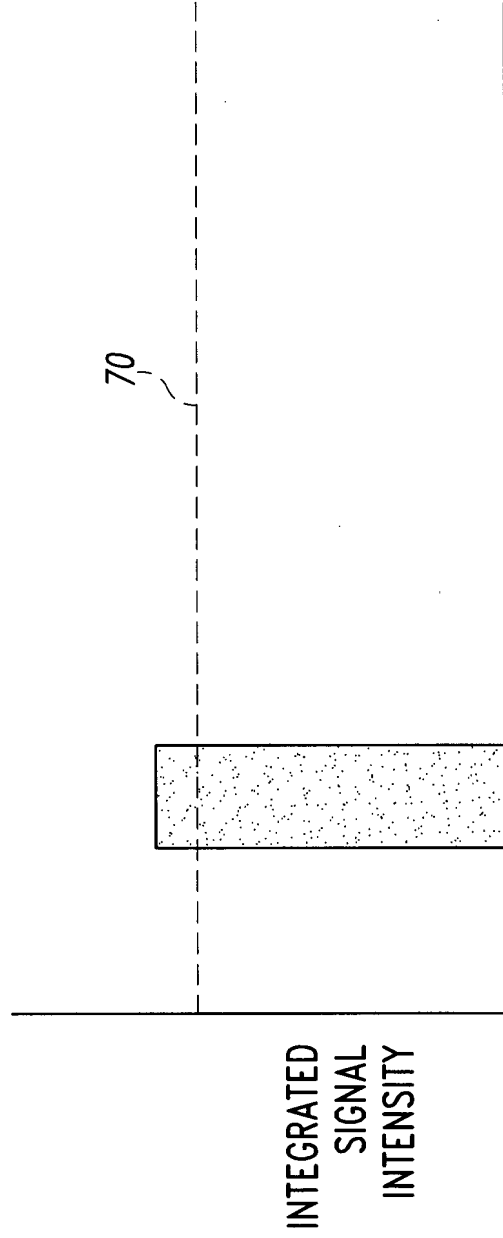


Fig. 8

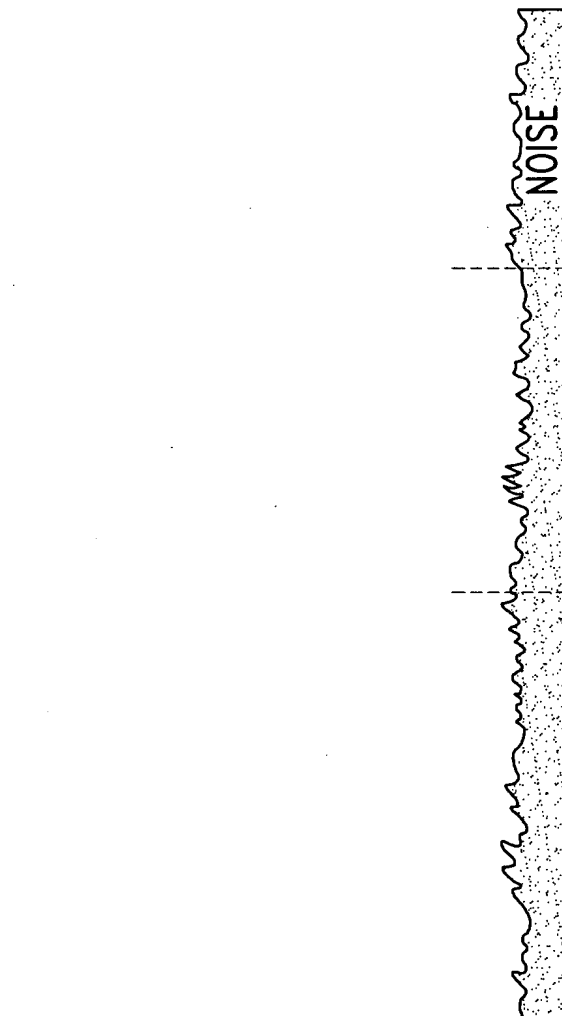


Fig. 9

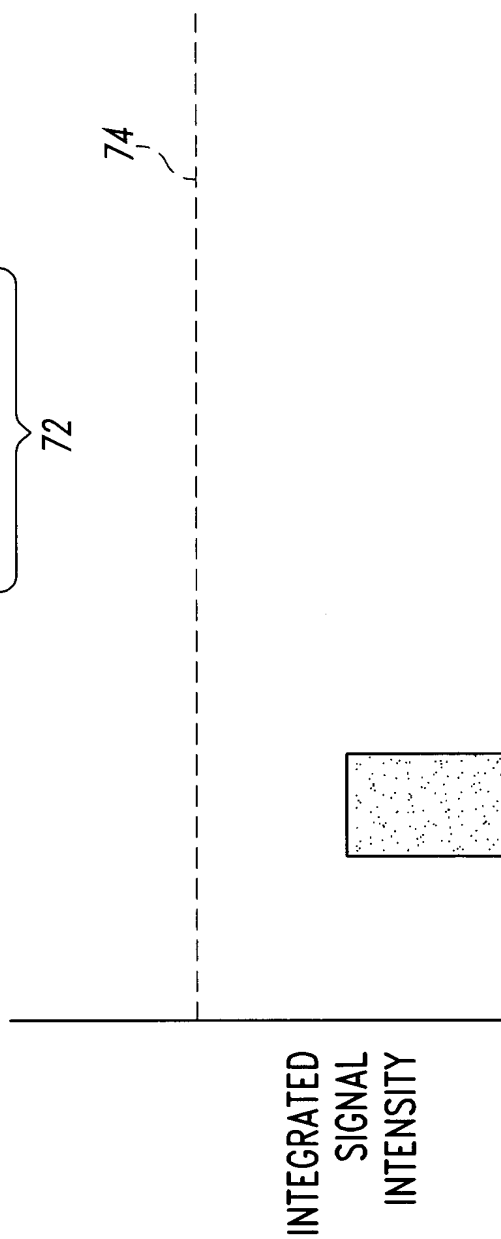


Fig. 10

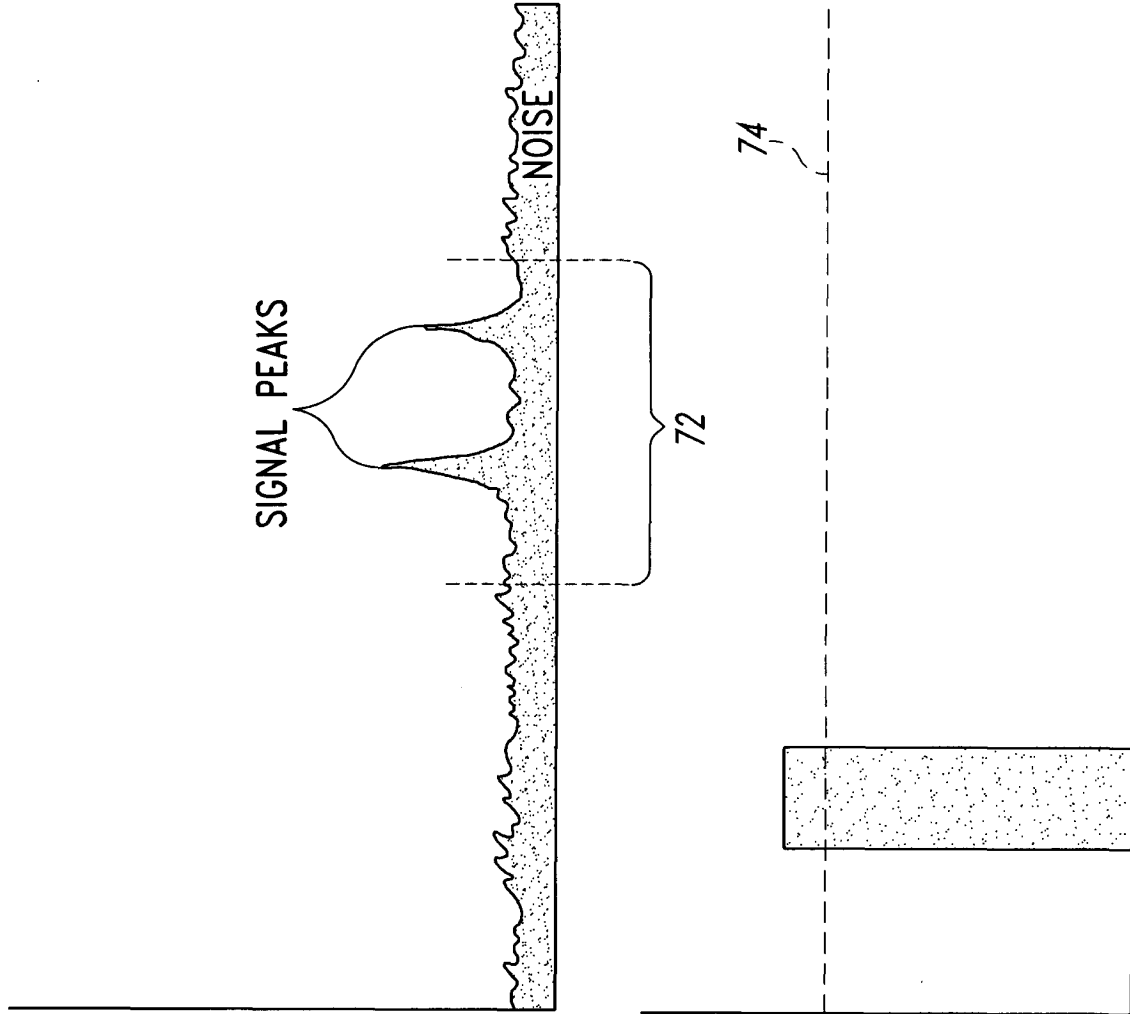


Fig. 11

INTEGRATED
SIGNAL
INTENSITY

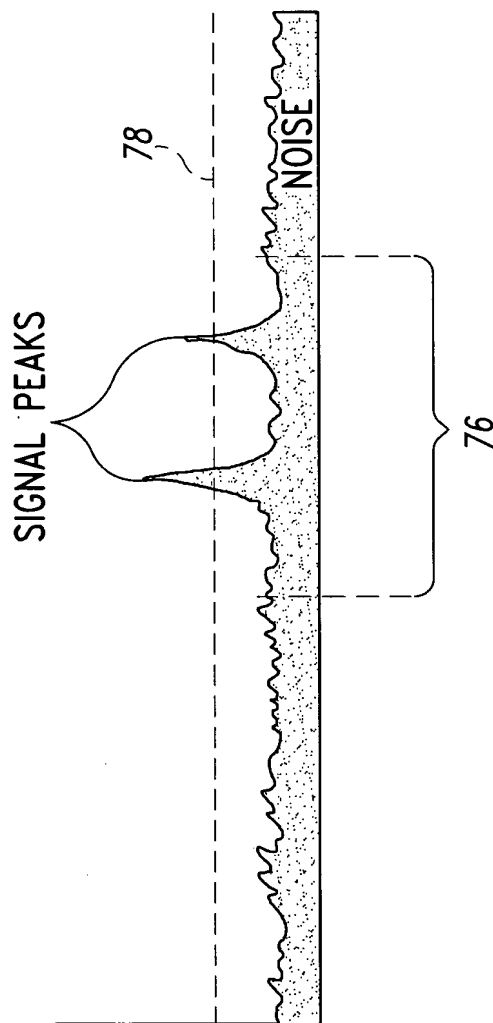


Fig. 12

METHOD AND APPARATUS FOR
CONTROLLING POSITION OF A LASER
OF A MALDI MASS SPECTROMETER

James P. Reilly et al.
32993-72728/ARTI-0335-A

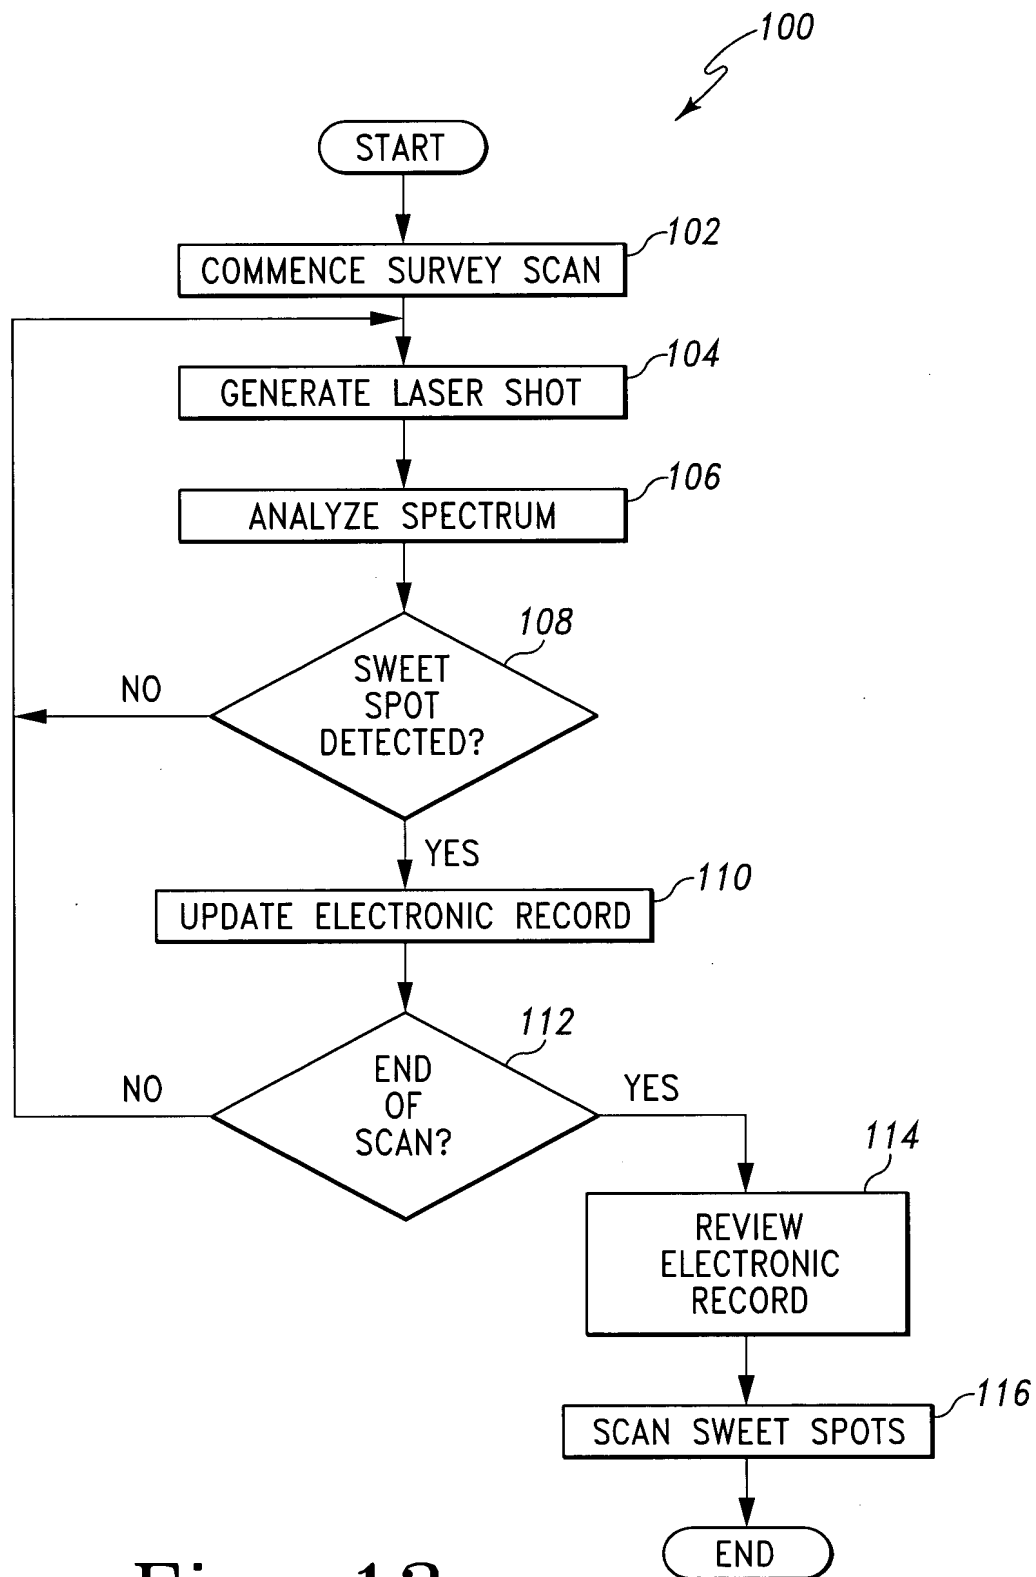


Fig. 13

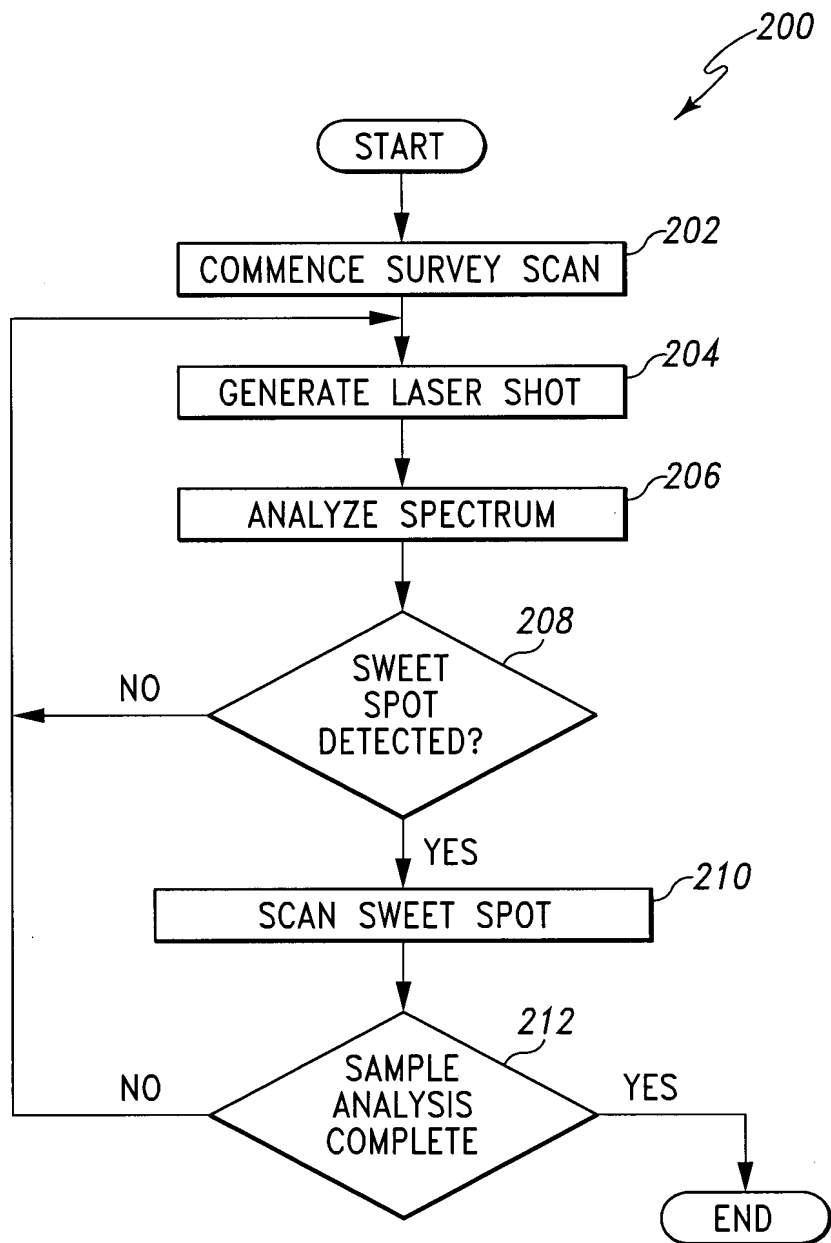


Fig. 14